

APPLICATIONS

Balancing Selectivity, Retention and Method Run Time of Two HPLC and UHPLC Particle Architectures

Zeshan Aqeel and J Preston
Phenomenex, Inc., 411 Madrid Ave., Torrance, CA 90501 USA

Overview

In order to achieve higher sensitivity, the use of sub-2 μm and high-pressure instruments to maximize performance has increased. Also, the increase in availability of different sub-2 μm particle architectures, allows for the selection of a particle and bonding ligand that balances the required method results. In this application, we investigate the balance of retention and method run time, with respect to particle architecture or morphology. The comparison below includes two of our most popular particle morphologies, the Kinetex Core-Shell and Luna Omega Thermally Modified Fully Porous UHPLC products. The sample was a general selectivity probe mix that combines seven different compounds of different classification – acidic, basic, and neutral compounds.

- Two Particle Morphologies
- Fully Scalable – HPLC to UHPLC
- High Performance & Reproducibility

LC Conditions

Column: Luna[®] Omega 1.6 μm C18
Kinetex[®] 1.7 μm C18

Dimension: 50 x 2.1 mm

Part No.: [00B-4742-AN](#)
[00B-4475-AN](#)

Mobile Phase: A: Water with 0.1 % Formic Acid
B: Acetonitrile with 0.1 % Formic Acid

Gradient:	Time (min)	B %
	0	5
	0.5	5
	5.5	95
	6.5	95
	7.0	5
	9.0	5

Flow Rate: 5.0 mL/min


Temperature: 30 °C

Detector: UV @ 256 nm

Injection Volume: 0.3 μL (5 $\mu\text{g}/\text{mL}$)

Sample: 1. Uracil
2. Pindolol
3. Chlorpheniramine
4. Nortriptyline
5. 3-Methyl-4-Nitrobenzoic Acid
6. 2-Hydroxy-5-Methylbenzaldehyde
7. Hexanophenone


Luna Omega 1.6 μm C18 Three Batch Comparison:

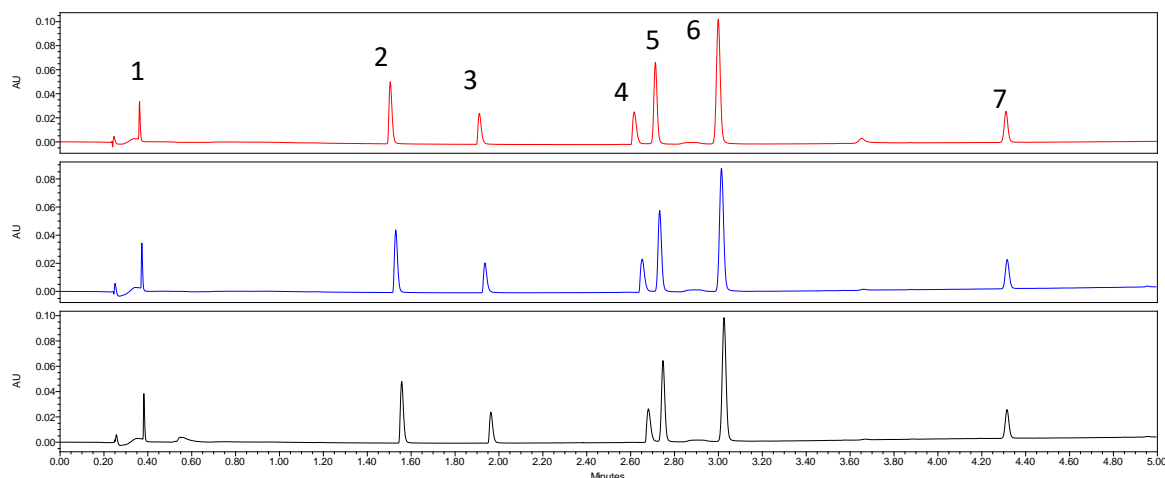

App ID: 26107

Retention and Selectivity Overlay

This overlay was generated at the same time and using the same standard mixture dissolved in water with 0.1 % formic acid. A 0.5 µL injection volume of 5 µg/mL standard solution was used in all examples. The same Waters® ACQUITY® I-Class instrument and chromatographic conditions were used in all examples.

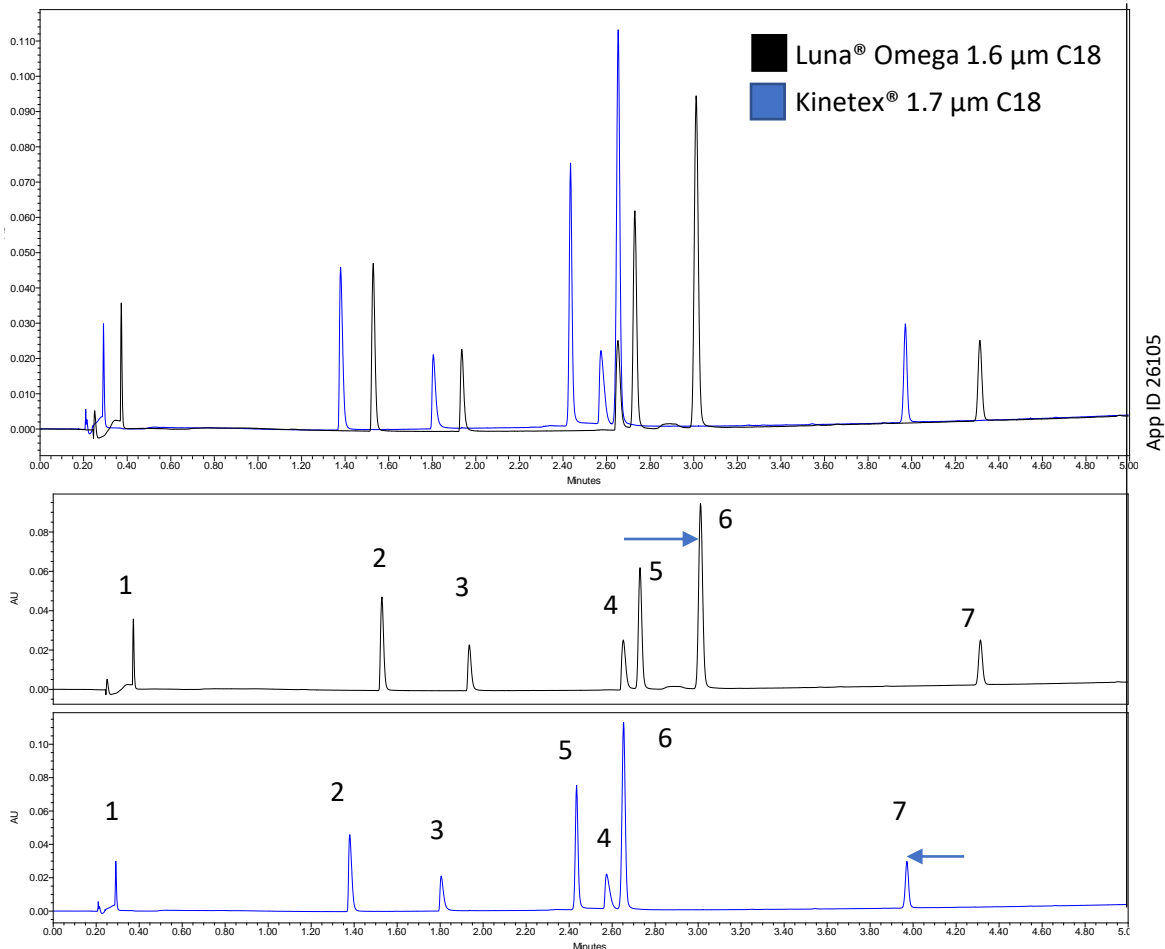

Conclusion

Both the Luna Omega and Kinetex C18 portrayed broad compound selectivity and retention with a diverse mixture of seven representative selectivity probes. The Kinetex 1.7 µm C18 demonstrated an overall faster runtime in comparison to the more retentive Luna Omega 1.6 µm C18. However, retention difference also alludes to a slight difference in selectivity, and in the case of peaks 4 and 5, a reversal of compound elution order under the same chromatographic conditions. Therefore, allowing method developers two options that help narrow down selection of a particle architecture and phase selectivity that most apparently fits the analytical demands of their method. Starting your initial method investigation with Luna Omega 1.6 µm and Kinetex 1.7 µm C18 ensures you are starting on both a fully UHPLC to HPLC scalable and batch-to-batch reproducible column particle platform.

APPLICATIONS

Need a different column size or sample preparation format?

No problem! We have a majority of our available dimensions up on www.phenomenex.com, but if you can't find what you need right away, our super helpful Technical Specialists can guide you to the solution via our online chat portal www.phenomenex.com/LiveChat.

<p>Australia t: +61 (0)2-9428-6444 auinfo@phenomenex.com</p>	<p>India t: +91 (0)40-3012 2400 indiainfo@phenomenex.com</p>	<p>Portugal t: +351 221 450 488 ptinfo@phenomenex.com</p>
<p>Austria t: +43 (0)1-319-1301 anfrage@phenomenex.com</p>	<p>Ireland t: +353 (0)1 247 5405 eirinfo@phenomenex.com</p>	<p>Singapore t: +65 800-852-3944 sginfo@phenomenex.com</p>
<p>Belgium t: +32 (0)2 503 4015 (French) t: +32 (0)2 511 8666 (Dutch) beinfo@phenomenex.com</p>	<p>Italy t: +39 051 6327511 italiainfo@phenomenex.com</p>	<p>Spain t: +34 91-413-8613 espinfo@phenomenex.com</p>
<p>Canada t: +1 (800) 543-3681 info@phenomenex.com</p>	<p>Luxembourg t: +31 (0)30-2418700 nlinfo@phenomenex.com</p>	<p>Sweden t: +46 (0)8 611 6950 nordicinfo@phenomenex.com</p>
<p>China t: +86 400-606-8099 cninfo@phenomenex.com</p>	<p>Mexico t: 01-800-844-5226 tecnicomx@phenomenex.com</p>	<p>Switzerland t: +41 (0)61 692 20 20 swissinfo@phenomenex.com</p>
<p>Denmark t: +45 4824 8048 nordicinfo@phenomenex.com</p>	<p>The Netherlands t: +31 (0)30-2418700 nlinfo@phenomenex.com</p>	<p>Taiwan t: +886 (0) 0801-49-1246 twinfo@phenomenex.com</p>
<p>Finland t: +358 (0)9 4789 0063 nordicinfo@phenomenex.com</p>	<p>New Zealand t: +64 (0)9-4780951 nzinfo@phenomenex.com</p>	<p>United Kingdom t: +44 (0)1625-501367 ukinfo@phenomenex.com</p>
<p>France t: +33 (0)1 30 09 21 10 franceinfo@phenomenex.com</p>	<p>Norway t: +47 810 02 005 nordicinfo@phenomenex.com</p>	<p>USA t: +1 (310) 212-0555 info@phenomenex.com</p>
<p>Germany t: +49 (0)6021-58830-0 anfrage@phenomenex.com</p>	<p>Poland t: +48 22 104 21 72 pl-info@phenomenex.com</p>	<p>🌐 All other countries/regions Corporate Office USA t: +1 (310) 212-0555 info@phenomenex.com</p>

www.phenomenex.com

Phenomenex products are available worldwide. For the distributor in your country/region, contact Phenomenex USA, International Department at international@phenomenex.com

BE-HAPPY[™]
guarantee

Your happiness is our mission. Take 45 days to try our products. If you are not happy, we'll make it right.

www.phenomenex.com/behappy

Terms and Conditions

Subject to Phenomenex Standard Terms and Conditions, which may be viewed at www.phenomenex.com/TermsAndConditions.

Trademarks

Luna and Kinetex are registered trademarks and BE-HAPPY is a trademark of Phenomenex. Waters and ACQUITY are registered trademarks of Waters Technologies Corporation. Phenomenex is not affiliated with Waters Corporation.

FOR RESEARCH USE ONLY. Not for use in clinical diagnostic procedures.

© 2020 Phenomenex, Inc. All rights reserved.