

APPLICATIONS

Quantitation of Human Plasma and Breast Milk Thiamine Monophosphate (TMP) and Thiamine by Applying ImpactTM Protein Precipitation Plate Technology with Gemini[®] 3 μ m NX-C18 HPLC Columns

Shuguang Li, Seyed Sadjadi, Sky Countryman, and Erica Pike
Phenomenex, Inc., 411 Madrid Ave., Torrance, CA 90501 USA

Thiamine monophosphate (TMP) and thiamine were extracted from human plasma and human breast milk by performing a rapid protein precipitation using Impact Protein Precipitation Plates followed by HPLC analysis using a Gemini 3 μ m NX-C18 100 x 3.0 mm HPLC column with fluorescence detection. Impact technology offers easy, fast protein removal while providing maximized recovery of the target analytes. The Gemini 3 μ m NX-C18 HPLC column produced excellent chromatographic resolution, sensitivity, and high peak capacities.

Introduction

Vitamin B1, also known as thiamine, is mainly present in human body fluids and tissue as thiamine diphosphate (TDP), thiamine monophosphate (TMP) and free thiamine. TDP, the most abundant thiamine derivative, is well described as a cofactor of several important enzymes, whereas TMP and thiamine are thought to be simple intermediates for which no specific role has currently been defined. TDP is commonly monitored from whole blood while TMP has reportedly shown higher concentrations in cerebrospinal fluids as compared to TDP. For this reason, it is important that analysis techniques be both sensitive and accurate.

Materials and Methods

Protein Precipitation

96-Well Plate: Impact Protein Precipitation Plate (Part No.: CE0-7565)

Part No.: CE0-7565

Dispense: 100 μ L of human plasma or breast milk into each well of the Impact plate

Add: 300 μ L of methanol to each well of the Impact plate

Mix: 3 times by aspirating with a pipette tip

Apply: Vacuum to filter the sample and collect the purified filtrate in a collection plate

Transfer 50 μ L to an autosampler vial (or allow it to remain in the collection plate). Add 50 μ L of water and 50 μ L of derivatizing reagent (15% sodium hydroxide solution plus 200 μ L of 30 mM $K_3Fe(CN)_6$). Cover the vial or collection plate with a lid or sealing mat, respectively. Vortex for 15 seconds. Put the vial or collection plate into an autosampler. The sample is now ready to be injected onto the HPLC-FLD.

HPLC Conditions

An Agilent[®] 1100 HPLC system (Agilent Technologies, Inc., Santa Clara, CA, USA) was used with a Shimadzu[®] RF-20A Prominence[®] Fluorescence Detector (Shimadzu, Japan) for LC/FLD analysis.

Column:	Gemini NX-C18 3 μ m	
Dimensions:	100 x 3.0 mm	
Part No.:	00D-4453-Y0	
Mobile Phase:	A: 25 mM Na_2HPO_4 , 10% Methanol (pH 7.0) B: 25 mM Na_2HPO_4 , 70% Methanol (pH 7.0)	
Gradient:	Time (min)	% A
	0.0	3
	0.25	25
	0.75	25
	3.00	35
	4.00	100
	5.00	100
	5.10	3
	8.00	3
Flow Rate:	750 μ L	
Detection:	Fluorescence (Excitation: 375 nm, Emission: 435 nm)	
Temperature:	25 $^{\circ}$ C	
Injection:	20 μ L	

Figure 1.
Protein Precipitation Using Impact Protein Precipitation Plates


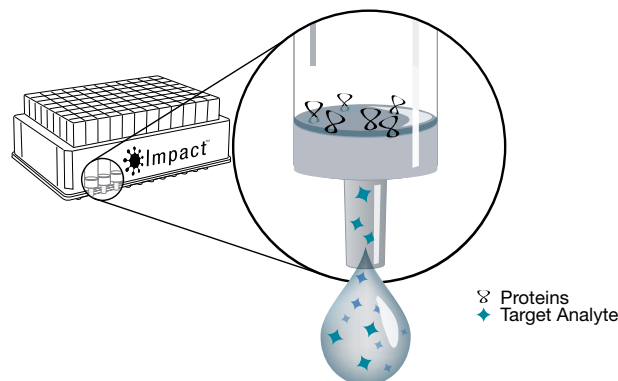


Figure 2.
200 nmol/L of TMP and thiamine in water filtered by an Impact Protein Precipitation Plate

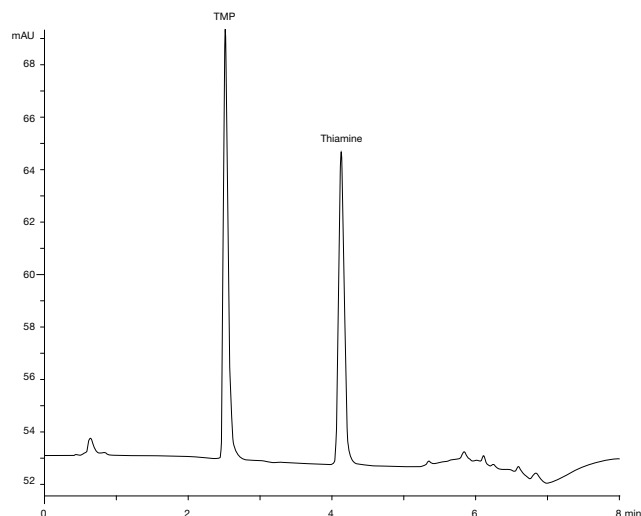

APPLICATIONS

Figure 3a.
2.5 nmol/L of TMP and thiamine in water filtered by an Impact Protein Precipitation Plate

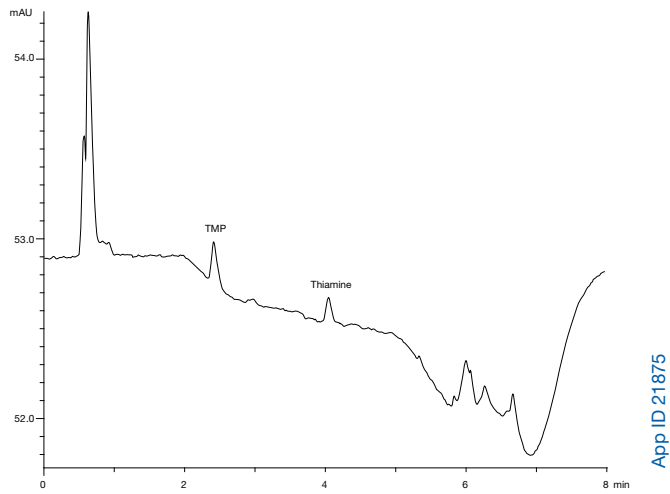


Figure 3b.
Comparison of TMP and thiamine at 25 nmol/L vs. blank control (overlay and expanded chromatograms for human plasma filtered by an Impact Protein Precipitation Plate)

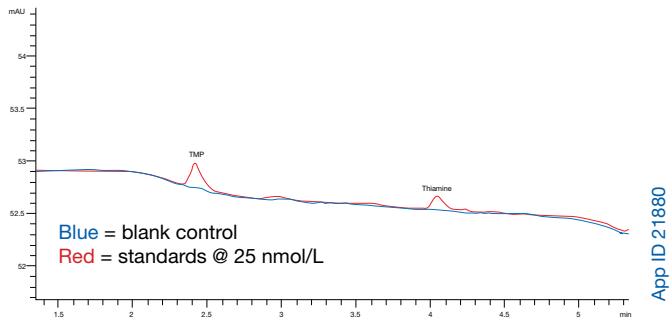


Figure 4.
Higher level TMP (93.6 nmol/L) and thiamine (240.8 nmol/L) in human breast milk

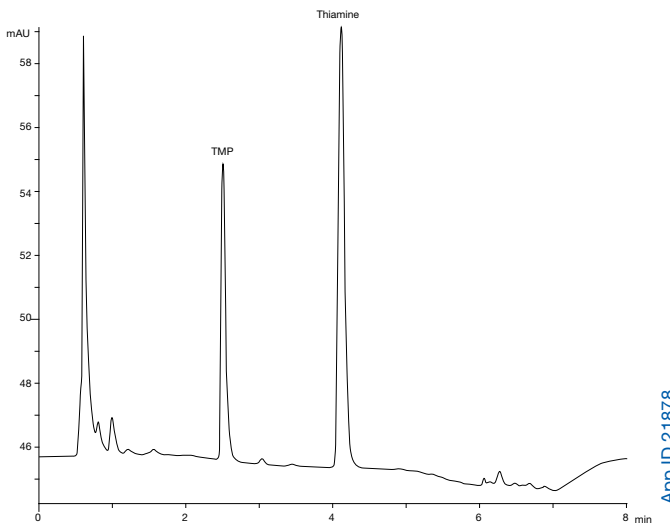


Figure 5.
Lower level TMP (37.2 nmol/L) and thiamine (66.4 nmol/L) in human breast milk

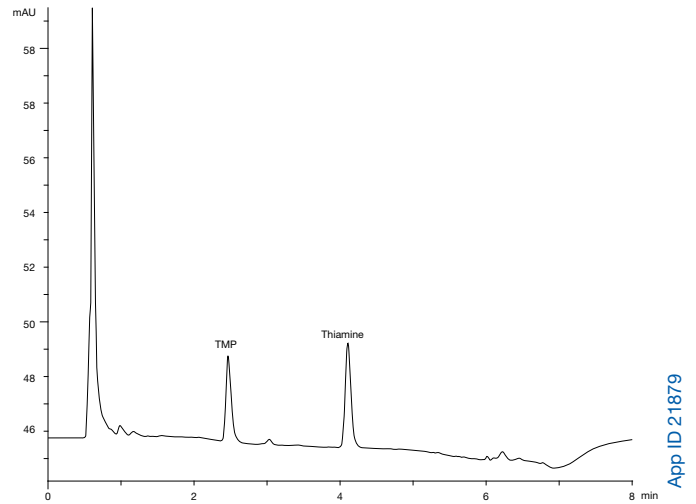


Figure 6.
Standard curve of TMP filtered by an Impact Protein Precipitation Plate at a concentration range of 0 to 200 nmol/L

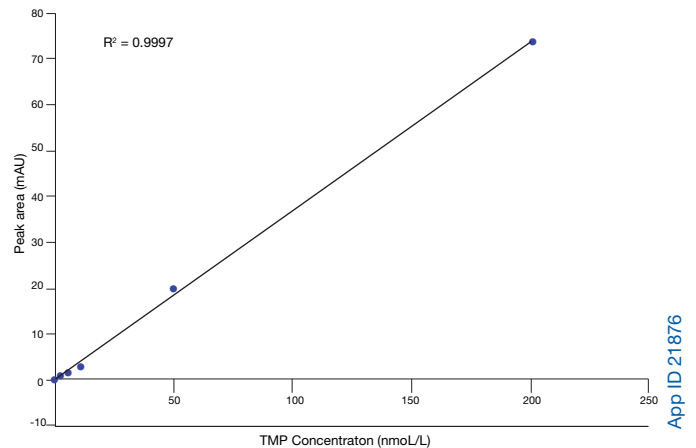


Table 1.
Standard curve (6-point) of TMP

TMP Standard Curve (6-point)	
Concentration (nmol/L)	Peak Area (mAU)
0	0
2.5	0.8
5	1.5
10	3.1
50	19.4
200	73.6

Table 2.
Recovery of TMP and thiamine from human plasma after cleanup with an Impact Protein Precipitation Plate


Recovery for Human Plasma TMP			Recovery for Human Plasma Thiamine		
Added TMP (nmol/L)	Observed (nmol/L)	Recovery (%)	Added Thiamine (nmol/L)	Observed (nmol/L)	Recovery (%)
0	3.0		0	5.0	
5	7.0	87.5	5	10.8	108.0
10	12.8	98.5	10	18.4	122.7
	Mean	93.0		Mean	115.4

APPLICATIONS

Table 3.
Accuracy studies for TMP and thiamine from human plasma after cleanup with an Impact Protein Precipitation Plate

Control No.	TMP Spiked Plasma Controls			Thiamine Spiked Plasma Controls		
	Expected (nmol/L)	Results (nmol/L)	Accuracy (%)	Expected (nmol/L)	Results (nmol/L)	Accuracy (%)
Control 1	40	38.7	96.8	40	34.2	85.5
Control 2	20	20.0	99.8	20	19.9	99.4
Control 3	10	10.7	107.0	10	8.2	81.8
		Mean	101.2		Mean	88.9

Figure 7.
Overlay of endogenous and spiked TMP and thiamine in plasma filtered by Impact

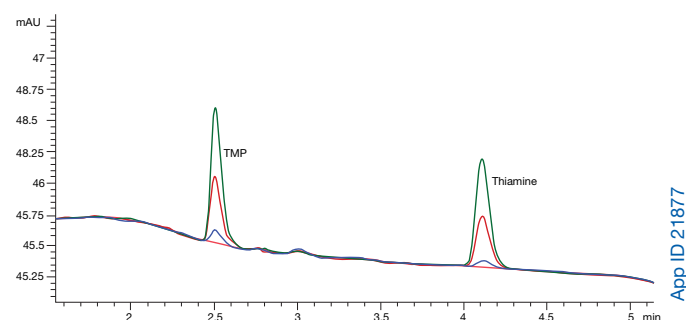

Blue = endogenous TMP (3 nmol/L) and thiamine (5 nmol/L)
 Red = spiked TMP (5 nmol/L) and thiamine (5 nmol/L)
 Green = spiked TMP (10 nmol/L) and thiamine (10 nmol/L)

Table 4.
Retention time reproducibility studies

Inj. No.	Retention Time (RT)	
	TMP (min)	Thiamine (min)
100	2.487	4.032
150	2.534	4.133
180	2.528	4.143
240	2.491	4.122
400	2.411	4.045
420	2.452	4.061
490	2.44	4.04
Mean	2.4818	4.0822
STEDV	0.0393	0.0483
%CV	1.58	1.18

Results and Discussion

When developing a method for the analysis of TMP and thiamine, it was important that the method be rapid, sensitive, and accurate in order to accommodate high-throughput labs that analyze 100's to 1000's of samples each week. Traditionally, a protein precipitation step is used for fast cleanup of plasma or breast milk samples. Protein precipitation is normally performed using a centrifuge tube or a 96-well collection plate; however this process requires that supernatant be collected while being careful not to disrupt pelleted protein in the bottom of the tube or collection plate. This step was greatly simplified by using Impact Protein Precipitation Plates. The Impact plate allows for the analysis of 96

samples at once, eliminates the transfer steps that are commonly associated with protein precipitation, and can also be automated. Protein precipitation was performed within the wells of the Impact plate and sample was not allowed to pass through the filter of the plate until vacuum was applied. This ensured that the precipitated protein was left within the wells of the Impact plate while protein free sample was allowed to pass through the filter and into a collection plate (**Figure 1**).

After the protein precipitation step, the plasma and breast milk samples were derivatized and analyzed by HPLC-FLD using a Gemini[®] 3 μ m NX-C18 HPLC column. The Gemini 3 μ m NX-C18 HPLC column contains a unique silica-organic layer that is grafted onto the base silica which mechanically strengthens the particle while providing excellent efficiencies. Efficiency and resolution were necessary in this analysis because the separation of TMP and thiamine (**Figures 2, 3a, and 3b**) was crucial in order to accurately quantify each compound in plasma (**Figure 7**) and breast milk (**Figures 4 and 5**).

The reproducibility of our analysis was determined by producing a standard curve of TMP at a concentration range of 0 to 200 nmol/L, resulting in a correlation coefficient of $R^2 = 0.9997$ (**Figure 6**). Thiamine was also subjected to a linearity curve at a concentration range of 0 to 200 nmol/L, resulting in a correlation coefficient of $R^2 = 0.9993$ (not shown). Even at low levels of detection, our method proved to be reproducible for both TMP and thiamine.

Compared with a water blank, the lower level TMP and thiamine standards (2.5 nmol/L) can be clearly distinguished (**Figure 3b**), showing that our extraction and HPLC method are extremely sensitive. Endogenous levels of TMP and thiamine were also studied in plasma (**Figure 7**), which showed that 3 nmol/L and 5 nmol/L were present, respectively.

Resulting recoveries of both target compounds averaged 93 % for human plasma TMP and 115 % for thiamine (**Table 2**). Accuracy studies resulted in an average accuracy of 101.2 for TMP and 88.9 for thiamine (**Table 3**), suggesting that our method not only provided acceptable recoveries but was also accurate and reproducible.

Retention times (RT) were stable by comparing several retention times between injection number 100 and 490, resulting in % CV's of 1.58 % for TMP and 1.18 % for thiamine (**Table 4**).

Conclusion

With vitamin testing on the rise, laboratories must develop rapid, reliable, and robust analytical methods that can be easily incorporated into a high-throughput setting. Protein precipitation has always been a popular sample preparation method however the process can be improved upon. Using Impact Protein Precipitation Plates, TMP and thiamine were cleaned up from plasma and breast milk providing benefits such as minimal method development and processing time as well as ease of use. The resulting cleanup method can also be automated, allowing laboratories to save time by increasing productivity while improving reproducibility and reducing the risk of human error. Preparation by automated protein precipitation is also a versatile sample preparation technique as the resulting extract can be analyzed by several different methods including HPLC/UV, LC/MS/MS, and HPLC-FLD. Using HPLC-FLD, our separation method on the Gemini 3 μ m NX-C18 HPLC column provided excellent resolution of TMP and thiamine and was sensitive enough to detect down to low levels, making it applicable to clinical analysis.

APPLICATIONS

Ordering Information

Gemini[®] HPLC Columns

3 μ m Microbore, Minibore and Narrow Bore Columns (mm)

Phases	SecurityGuard [™] Cartridges (mm)								
	20 x 2.0	30 x 2.0	50 x 2.0	100 x 2.0	150 x 2.0	50 x 3.0	100 x 3.0	150 x 3.0	4 x 2.0*
NX-C18	00M-4453-B0	00A-4453-B0	00B-4453-B0	00D-4453-B0	00F-4453-B0	00B-4453-Y0	00D-4453-Y0	00F-4453-Y0	/10pk AJ0-8367

for ID: 2.0-3.0 mm

3 μ m Analytical Columns (mm)

Phases	SecurityGuard [™] Cartridges (mm)				
	50 x 4.6	100 x 4.6	150 x 4.6	250 x 4.6	4 x 3.0*
NX-C18	00B-4453-E0	00D-4453-E0	00F-4453-E0	00G-4453-E0	/10pk AJ0-8368

for ID: 3.2-8.0 mm

5 μ m Minibore and Narrow Bore Columns (mm)

Phases	SecurityGuard [™] Cartridges (mm)							
	30 x 2.0	50 x 2.0	150 x 2.0	50 x 3.0	100 x 3.0	150 x 3.0	250 x 3.0	4 x 2.0*
NX-C18	00A-4454-B0	00B-4454-B0	00F-4454-B0	00B-4454-Y0	00D-4454-Y0	00F-4454-Y0	00G-4454-Y0	/10pk AJ0-8367

for ID: 2.0-3.0 mm

5 μ m Analytical Columns (mm)

Phases	SecurityGuard [™] Cartridges (mm)				
	50 x 4.6	100 x 4.6	150 x 4.6	250 x 4.6	4 x 3.0*
NX-C18	00B-4454-E0	00D-4454-E0	00F-4454-E0	00G-4454-E0	/10pk AJ0-8368

for ID: 3.2-8.0 mm

Ordering Information

Impact[™] Protein Precipitation Plates

Part No.	Description	Unit
Impact Precipitation Plates		
CE0-7565	Impact Protein Precipitation, Square Well, Filter Plate, 2 mL	2/box

Impact Starter Kit for Protein Precipitation

CE0-8201	Impact Protein Precipitation Plate (2 ea) Collection Plate 2 mL (2 ea) Sealing Mat, Santoprene [™] (AH0-8199) (2 ea)	ea
----------	---	----

Accessories

Collection Plates (deep well, polypropylene)

AH0-7192	96-Well Collection Plate 350 μ L/well	50/pk
AH0-7193	96-Well Collection Plate 1 mL/well	50/pk
AH0-7194	96-Well Collection Plate 2 mL/well	50/pk
AH0-8635	96-Well Collection Plate, 2 mL Square/Round-Conical	50/pk
AH0-8636	96-Well Collection Plate, 2 mL Round/Round, 8 mm	50/pk
AH0-7279	96-Well Collection Plate, 1 mL/well Round, 7 mm	50/pk

Sealing Mats

AH0-8597	Sealing Mats, Pierceable, 96-Square Well, Silicone	50/pk
AH0-8598	Sealing Mats, Pre-Slit, 96-Square Well, Silicone	50/pk
AH0-8631	Sealing Mats, Pierceable, 96-Round Well 7 mm, Silicone	50/pk
AH0-8632	Sealing Mats, Pre-Slit, 96-Round Well 7 mm, Silicone	50/pk
AH0-8633	Sealing Mats, Pierceable, 96-Round Well 8 mm, Silicone	50/pk
AH0-8634	Sealing Mats, Pre-Slit, 96-Round Well 8 mm, Silicone	50/pk
AH0-7362	Sealing Tape Pad	10/pk

Vacuum Manifolds

AH0-8950	96-Well Plate Manifold, Universal with Vacuum Gauge	ea
----------	---	----



If Phenomenex products in this technical note do not provide at least an equivalent separation as compared to other products of the same phase and dimensions, return the product with your comparative data within 45 days for a FULL REFUND.

Terms and Conditions

Subject to Phenomenex Standard Terms and Conditions which may be viewed at www.phenomenex.com/TermsAndConditions.

Trademarks

Gemini is a registered trademark, and SecurityGuard and Impact are trademarks of Phenomenex. Agilent is a registered trademark of Agilent Technologies, Inc. Santoprene is a trademark of Exxon Mobil Corp. Shimadzu and Prominence are registered trademarks of Shimadzu Corp.

Gemini is patented by Phenomenex. U.S. Patent No. 7,563,367

FOR RESEARCH USE ONLY. Not for use in clinical diagnostic procedures.

© 2018 Phenomenex, Inc. All rights reserved.

Australia

t: +61 (0)2-9428-6444
auiinfo@phenomenex.com

Austria

t: +43 (0)1-319-1301
anfrage@phenomenex.com

Belgium

t: +32 (0)2 503 4015 (French)
t: +32 (0)2 511 8666 (Dutch)
beinfo@phenomenex.com

Canada

t: +1 (800) 543-3681
info@phenomenex.com

China

t: +86 400-606-8099
cninfo@phenomenex.com

Denmark

t: +45 4824 8048
nordicinfo@phenomenex.com

Finland

t: +358 (0)9 4789 0063
nordicinfo@phenomenex.com

France

t: +33 (0)1 30 09 21 10
franceinfo@phenomenex.com

Germany

t: +49 (0)6021-58830-0
anfrage@phenomenex.com

India

t: +91 (0)40-3012 2400
indiainfo@phenomenex.com

Ireland

t: +353 (0)1 247 5405
eireinfo@phenomenex.com

Italy

t: +39 051 6327511
italiainfo@phenomenex.com

Luxembourg

t: +31 (0)30-2418700
nlinfo@phenomenex.com

Mexico

t: 01-800-844-5226
tecnicomx@phenomenex.com

The Netherlands

t: +31 (0)30-2418700
nlinfo@phenomenex.com

New Zealand

t: +64 (0)9-4780951
nzinfo@phenomenex.com

Norway

t: +47 810 02 005
nordicinfo@phenomenex.com

Portugal

t: +351 221 450 488
ptinfo@phenomenex.com

Singapore

t: +65 800-852-3944
sginfo@phenomenex.com

Spain

t: +34 91-413-8613
espinfo@phenomenex.com

Sweden

t: +46 (0)8 611 6950
nordicinfo@phenomenex.com

Switzerland

t: +41 61 692 20 20
swissinfo@phenomenex.com

United Kingdom

t: +44 (0)1625-501367
ukinfo@phenomenex.com

USA

t: +1 (310) 212-0555
info@phenomenex.com

All other countries Corporate Office USA

t: +1 (310) 212-0555
info@phenomenex.com

www.phenomenex.com

Phenomenex products are available worldwide. For the distributor in your country, contact Phenomenex USA, International Department at international@phenomenex.com